

THROMBOPHILIA MULTIPLEX REAL TIME PCR KIT B

(12 MUTATIONS)

Cat. No: 10R-20-12B

PRODUCT DESCRIPTION

In Thrombophilia, blood has an increased tendency to form potentially dangerous clots. Hereditary defects in one or more of the clotting factors can cause to excessive blood clot formation called thrombosis. Thrombophilia Multiplex Real Time PCR Kit includes; FII Prothrombin, FV Leiden, FV 1299, FV Cambridge, FV Y1702C, MTHFR 677, MTHFR 1298, MTR 2756, MTRR 66, FXIII Val34Leu, Beta-Fibrinogen 455 G>A and PAI-1 4G/5G mutations.

PRINCIPLE OF THE SYSTEM

During the PCR reaction, the DNA polymerase cleaves the probe at the 5' end and separates the reporter dye from the quencher dye only when the probe hybridizes perfectly to the target DNA. This cleavage results in the fluorescent signal which is monitored by Real-Time PCR detection system. An increase in the fluorescent signal (CT) is proportional to the amount of the specific PCR product.

PRODUCT SPECIFICATION

Each isolated DNA should be tested with Mix 1, Mix 2, Mix 3, Mix 4, Mix 5, Mix 6, Mix 7 and Mix 8. The kit provides reagents in a ready-to-use mastermix format which has been specifically adapted for 5' nuclease PCR. The test system is designed for use with sequence specific primers and probe (See table 1). The fluorescence of mutation analysis is FAM, HEX/JOE and Texas Red. Also each mastermix contains an internal control labelled with CY5 dye.

SYSTEM CONTENTS

Reagents	20 rxns
• TRP-12B Mix 1	400 µl
• TRP-12B Mix 2	400 µl
• TRP-12B Mix 3	400 µl
• TRP-12B Mix 4	400 µl
• TRP-12B Mix 5	400 µl
• TRP-12B Mix 6	400 µl
• TRP-12B Mix 7	400 µl
• TRP-12B Mix 8	400 µl
• Control DNA	60 µl

STORAGE

- All reagents should be stored at – 20 °C and dark.
- All reagents can be used until the expiration date on the box label.
- Repeated thawing and freezing (>4X) should be avoided, as this may reduce the sensitivity of the assay.

DNA EXTRACTION

Blood samples should be collected in appropriate sterile EDTA tubes and can be stored at +4°C up to one month. For more than one month specimen should be stored at -20°C. It is advised to gently mix the tube (with EDTA) after collection of blood to avoid coagulation.

Our system optimized according to SNPure Blood® and MN NucleoSpin® Blood. It is advised to elute DNA with **150 µl elution buffer** for better results.

MUTATION / DYE TABLE

Table 1 : Tubes – mutations - dyes.

Tubes	Mutations	Dyes
Mix 1	FII Wild Type	FAM
	FV Wild Type	HEX/JOE
	677 Wild Type	TEXAS RED
	Internal Control	CY5
Mix 2	FII Mutant Type	FAM
	FV Mutant Type	HEX/JOE
	677 Mutant Type	TEXAS RED
	Internal Control	CY5
Mix 3	1298 Wild Type	FAM
	FV 1299 Wild Type	HEX/JOE
	PAI -1 5G	TEXAS RED
	Internal Control	CY5
Mix 4	1298 Mutant Type	FAM
	FV 1299 Mutant Type	HEX/JOE
	PAI -1 4G	TEXAS RED
	Internal Control	CY5
Mix 5	FXIII Wild Type	FAM
	FV Cambridge Wild Type	HEX/JOE
	B-Fibrinogen Wild Type	TEXAS RED
	Internal Control	CY5
Mix 6	FXIII Mutant Type	FAM
	FV Cambridge Mutant Type	HEX/JOE
	B-Fibrinogen Mutant Type	TEXAS RED
	Internal Control	CY5
Mix 7	FV 1702 Wild Type	FAM
	MTR 2756 Wild Type	HEX/JOE
	MTRR 66 Wild Type	TEXAS RED
	Internal Control	CY5
Mix 8	FV 1702 Mutant Type	FAM
	MTR 2756 Mutant Type	HEX/JOE
	MTRR 66 Mutant Type	TEXAS RED
	Internal Control	CY5

PROCEDURE

- Different tubes should be prepared for each mix.
- Before starting work, mix the mastermixes gently by pipetting
- For each sample, pipet **20 µl mastermix*** with micropipets of sterile filter tips to each optical white strips or tubes.
- Add **5 µl (~10-100 ng) DNA** into each tube.
- Run with the programme shown below.

**Master mixes include HotStart Taq DNA Polymerase.*

PCR PROGRAMME

95 °C	5 Min.	Holding
95 °C	15 Sec.	30 Cycles
60 °C	1 Min.	

Fluorescent dyes are FAM, TEXAS RED, CY5 and HEX/JOE.

This system can use with:

ABI Prism® 7000/7300/7500/7900

Bio-Rad CFX96

DATA ANALYSIS

After the run is completed data are analysed using the software with HEX (JOE), TEXAS RED, CY5 and FAM dyes. The below results were studied with Bio-Rad CFX96.

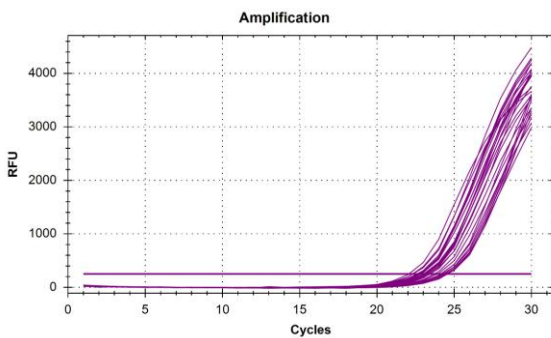


Figure 1: Internal Control plots – CY5 Dye

Internal control amplification plots must be seen in all wells except NTC and has been labelled with CY5 dye. The CT value of internal controls should be $21 \leq X \leq 26$.

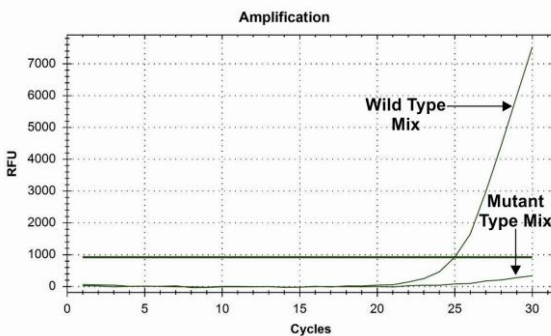


Figure 2: FV Wild Type – HEX Dye (Mix 1 – 2)

Amplification plots of mutations can be analysed by related dye*. The CT value should be between $21 \leq CT \leq 26$. These values are optimised according to the SNPure® Blood DNA Isolation Kit and MN NucleoSpin® Blood DNA Isolation Kit. CT values may vary $\pm 2/3$ cycle according to the DNA isolation protocol.

- Homozygote wild-type sample gives amplification signal only with wild-type mastermix.
- Heterozygote sample gives amplification signal both with wild-type and mutant mastermixes.

- Homozygote mutant sample gives amplification signal only with mutant mastermix.
- The difference of the CT value wild-type and mutant amplification plots should be ≤ 3 for heterozygote mutant sample. It is $4 \leq CT \leq 6$, test should be repeated.

*Please check tubes / mutations / dyes table (table 1).

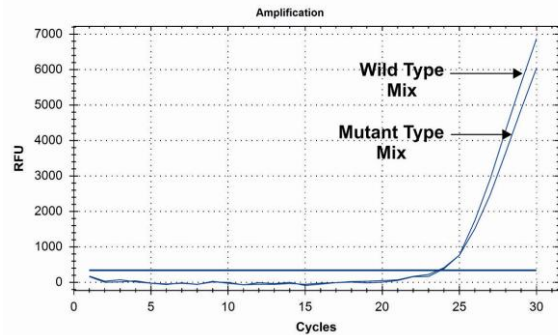


Figure 3: FXIII Heterozygote Type – FAM Dye (Mix 5 – 6)

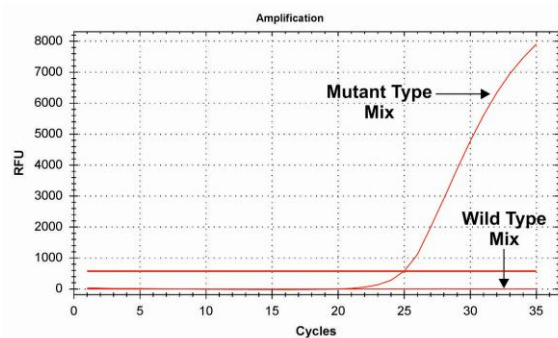


Figure 4: MTRR 66 Homozygote Mutant Type – TEXAS RED Dye (Mix 7 – 8)

TROUBLE SHOOTING

If internal control doesn't work,

- Absence of DNA
- Absence/Deficiency of Hot Start Taq DNA Polymerase
- Sample is containing DNA inhibitor(s)

If plots start late,

- DNA quality is not good.
- The amount of DNA is not enough.
- Sample is containing partial DNA inhibitor(s)

Please contact us for your questions. tech@snp.com.tr

CAUTIONS

- All reagents should be stored at suitable conditions.
- Do not use the PCR mastermixes forgotten at room temperature.
- Thaw PCR mastermix at room temperature and slowly mix by inverting before use.
- The PCR programme described above should be performed.
- Shelf-life of PCR mastermix is 12 months. Please check the manufacturing data before use.
- Only use in vitro diagnostics.